Flowflex® PLUS RSV + Flu A/B + COVID Home Test

Quick Reference Guide

PREPARATION

1 Wash — 2 Prepare — 3 Peel — 4 Place

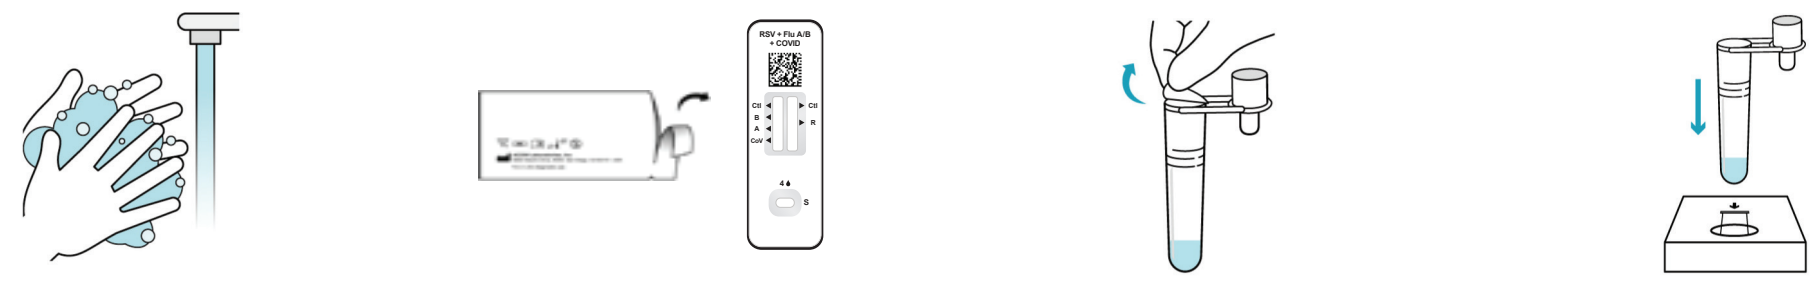

Proceed to steps for (6 months - 23 months) or (2 years and older)

TEST PROCEDURE FOR PEDIATRICS (6 MONTHS - 23 MONTHS)

1 Open — 2 Attach Guard — 3 Position Child — 4 Swab — 5 Swirl

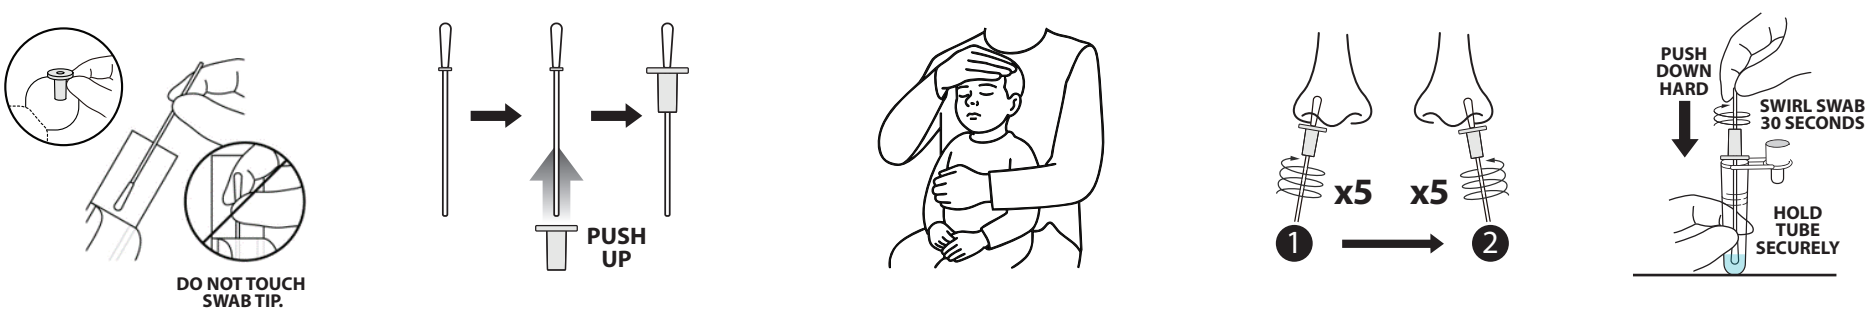

6 Rotate — 7 Remove — 8 Cap — 9 Drop — 10 Wait

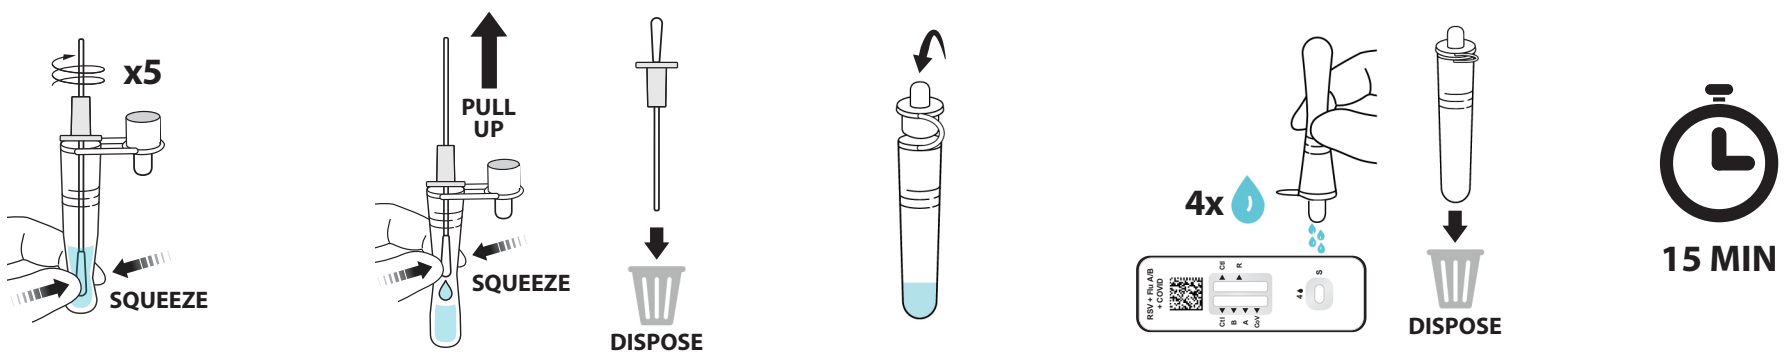

11 Read Results — 12 Dispose

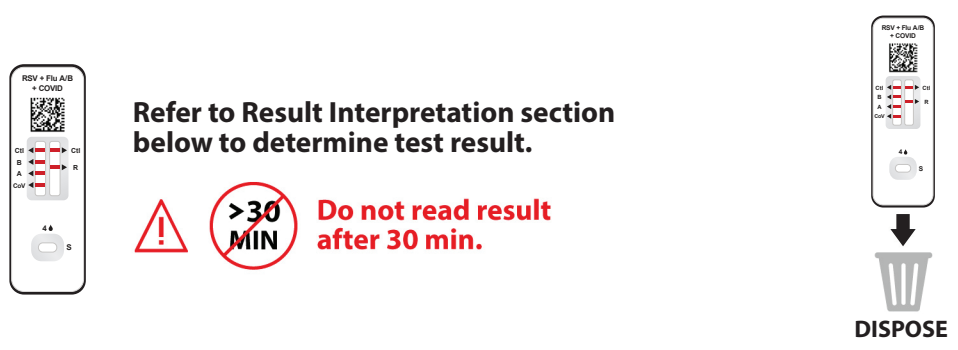

TEST PROCEDURE FOR 2 YEARS AND OLDER

1 Open — 2 Swab — 3 Swirl — 4 Rotate

5 Remove — 6 Cap — 7 Drop — 8 Wait

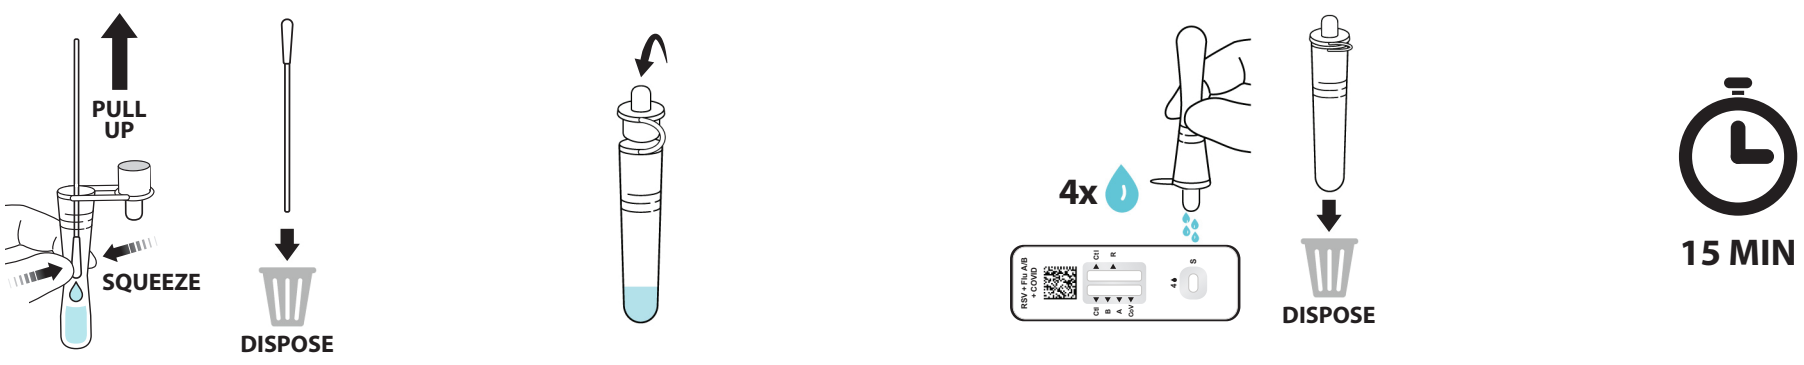

9 Read Results — 10 Dispose

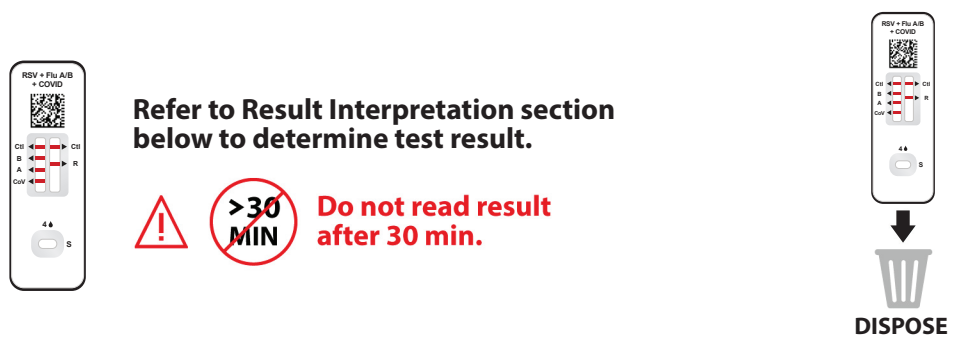

RESULT INTERPRETATION

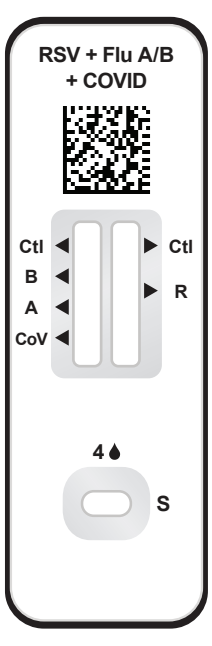

Negative



NEGATIVE RESULT

Invalid



INVALID RESULT



INVALID RESULT

Positive



COVID-19 POSITIVE



FLU A POSITIVE



FLU B POSITIVE



FLU A + FLU B POSITIVE



COVID-19 + FLU A POSITIVE



COVID-19 + FLU B POSITIVE



COVID-19 + FLU A + FLU B POSITIVE



RSV POSITIVE



COVID-19 + RSV POSITIVE



RSV + FLU A POSITIVE



RSV + FLU B POSITIVE



COVID-19 + FLU A + RSV POSITIVE



COVID-19 + FLU B + RSV POSITIVE



FLU A + FLU B + RSV POSITIVE



COVID-19 + FLU A + FLU B + RSV POSITIVE

Number: 1150003490
Effective Date: 12/17/2025

ACON Laboratories, Inc.
San Diego, CA 92121, USA
Customer Support 1-800-838-9502
flowflexcovid.com